
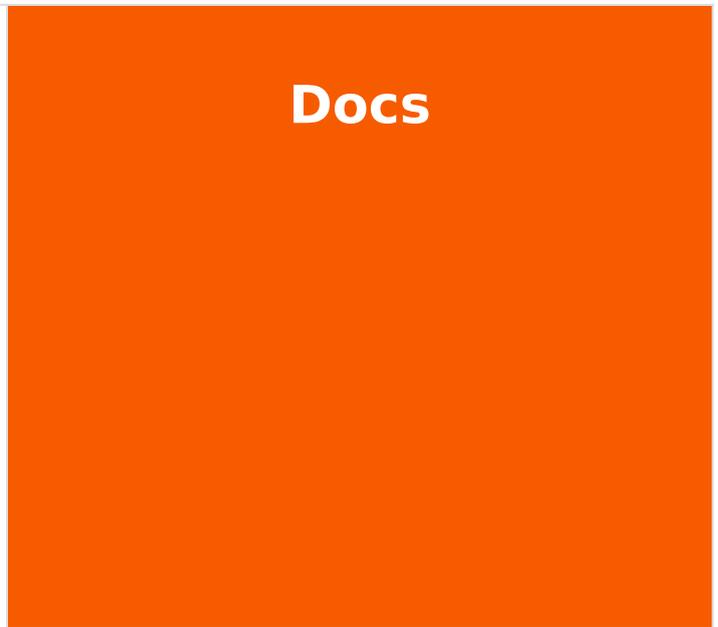


65.023 R4: Mouthwatch Intraoral camera setup for Carestream Dental - white screen

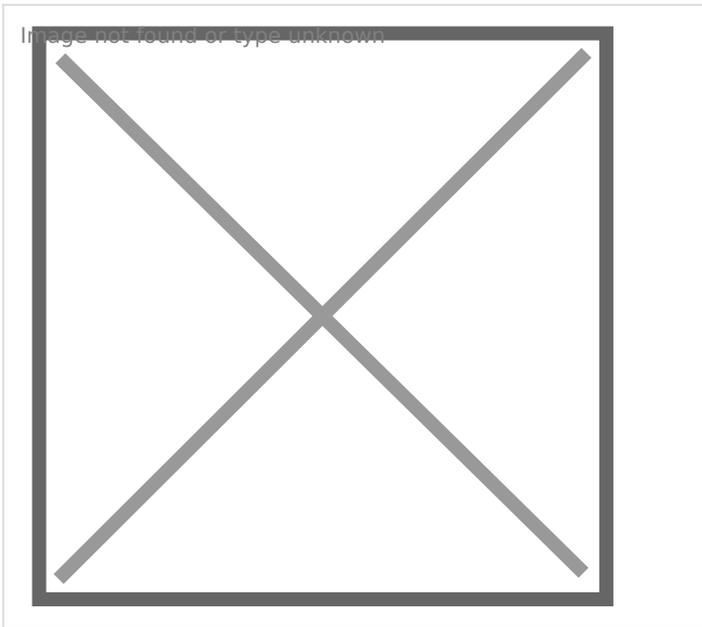

Document Control

Document Name	65.023 R4: Mouthwatch Intraoral camera setup for Carestream Dental - white screen		
Version	v1.0 Current		
Author	Neil Tancock, IT Services (Safeharbour Support Ltd), neil@safeharboursupport.com		
Approval	Safeharbour Support		
Approval date	01-JAN-2025	Review date	31-DEC-2027
Abstract	Sometimes a Windows update will knock out the ability for Kodak Imaging to pick up the video feed from a Mouthwatch camera and you get a white screen.		
Scope	This document applies to all clients of Safeharbour Support Ltd		
Inputs	None		

Outputs	None
----------------	------

Change Control

Date	Author	Version	Change
02-DEC-2024	Neil Tancock	0.0	First version
01-JAN-2025	Neil Tancock	1.0	Approved


-----<START OF DOCUMENT>-----

Sometimes a Windows update will knock out the ability for Kodak Imaging to pick up the video feed from a Mouthwatch camera and you get a white screen.

To fix this, you need to apply a registry update to windows:

- Open File Explorer and browse to "C:\Program Files (x86)\MouthWatch Capture\Files\Dentrix Image Fixes"

Image not found or type unknown



- If you are on a x64 machine, double click on whitescreenfix_x64.reg and confirm the registry update
- If you are on a x86 machine, double click on whitescreenfix_x86.reg and confirm the registry update

That's it! The video preview should now be working.

-----<END OF DOCUMENT> -----


Need help? Get in touch!

You can call us on [01752 373000](tel:01752373000), option 2 or, if you are on Number Club, just call extension 3001

You can email us at hub@safeharboursupport.com

You can chat & Collaborate with us at <https://kite.wildix.com/nc-a12/3001>

You can Whatsapp us right here: <https://wa.me/441752373000>



Revision #2

Created 20 February 2025 20:49:47 by Neil Tancock

Updated 20 February 2025 20:50:36 by Neil Tancock